


## The effect of ionic strength of the mobile phase additive for HPLC columns in Aqueous Normal Phase - Tips & Suggestions

### Ionic strength of additives can affect your retention times.

Ionic strength has a smaller or lesser effect in Cogent TYPE-C™ columns when used in Aqueous Normal Phase (ANP) than in methods with HILIC columns because the ANP mechanism is a type of "competitive adsorption" in the adsorbed layer with Acetonitrile, on the silica-hydride surface.

Ionic strength would be expected to have some impact on this processes. Using a lower amount of buffer agents such as formic acid with optimal retention can be a large advantage to using ANP methods. The charts below show examples of 4 compounds and the effect of formic acid in the mobile phase on retention.

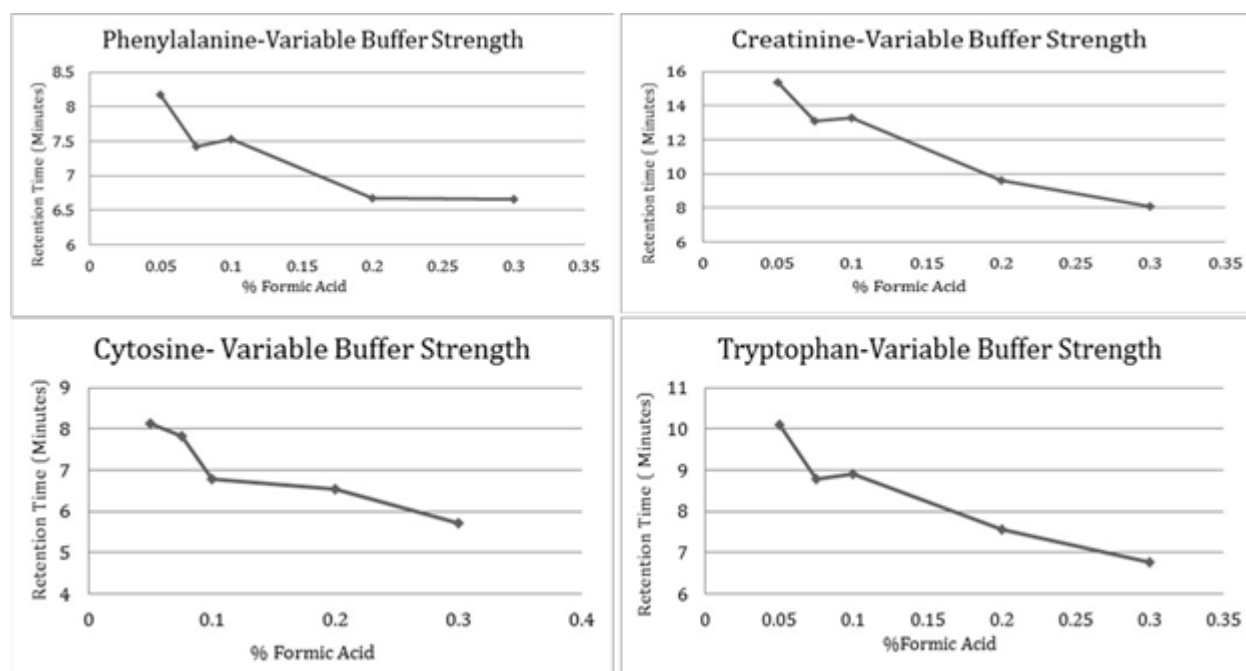

Printed from the Chrom Resource Center

Copyright 2025, All Rights Apply

**MicroSolv Technology Corporation**

9158 Industrial Blvd. NE, Leland, NC 28451

Tel: (732) 380-8900

Fax: (910) 769-9435

Email: [customers@mtc-usa.com](mailto:customers@mtc-usa.com)

Website: [www.mtc-usa.com](http://www.mtc-usa.com)