
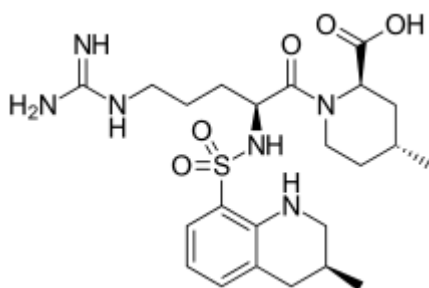


Argatroban analyzed with HPLC - AppNote

A simple method for this di-peptide

A rapid, sensitive, and reproducible method has been developed for this blood thinner. The data below, (an overlay of 10 chromatograms) illustrates how the compound can be adequately retained and detected using this straightforward method.

A phenyl ring in the column stationary phase provides strategic use of π - π Interaction with the analyte making possible the use of a very simple, Mass Spec-friendly mobile phase with formic acid as an additive.

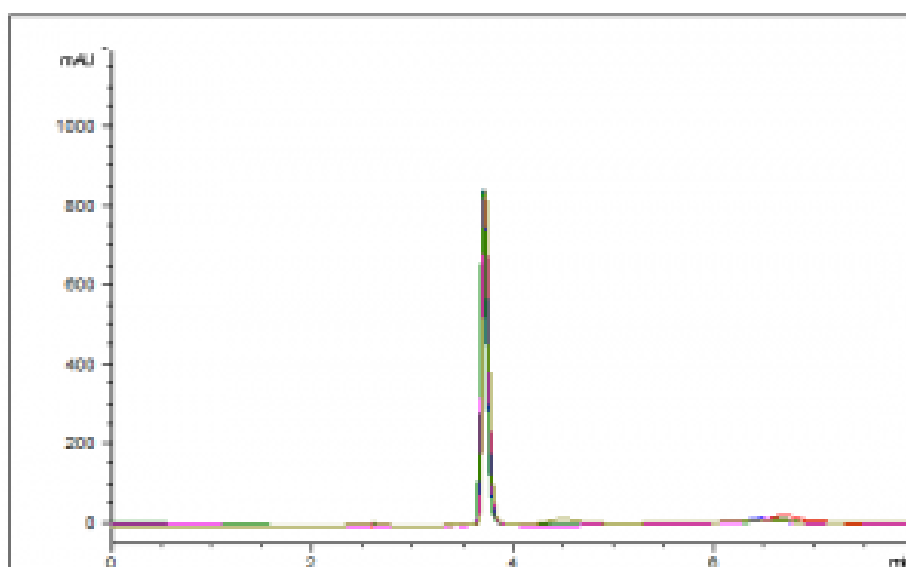

Peak:

Argatroban

Method Conditions

Column: Cogent Phenyl Hexyl™, 4μm, 100Å

Catalog No.: [68539-15P](#)

Dimensions: 4.6mm x 150mm

Mobile Phase:

A: DI water
B: Acetonitrile

Time (minutes)	%B
0	25
1	25
3	50
4	50
5	25
8	25

Injection vol.: 2µL

Flow rate: 1.0mL / minute

Detection: UV @ 215nm

Sample Preparation: 0.5 mg / mL in 50:50 acetonitrile / DI water

%RSD: <1.0%

t₀: 1.5 minutes

K': 1.35

Notes: Argatroban is a synthetic direct thrombin inhibitor used for the prevention and treatment of thrombosis related to heparin use. It acts as a preventative of the formation of blood clots, which reduces the risk for stroke or other medical conditions.

Note 2: Capacity is determined using the following equation: $k = (t_R - t_0) / t_0$

- t_R = Retention time of an analyte peak
- t_0 = Retention time of non-retained peak



Printed from the Chrom Resource Center
Copyright 2025, All Rights Apply
MicroSolv Technology Corporation
9158 Industrial Blvd. NE, Leland, NC 28451

Tel: (732) 380-8900
Fax: (910) 769-9435
Email: customers@mtc-usa.com
Website: www.mtc-usa.com