



## How does efficiency in Aqueous Normal Phase ANP compare to HILIC in HPLC - FAQ

**Aqueous Normal Phase ANP HPLC is a distinctly different retention mode than Hydrophilic Interaction Liquid Chromatography or HILIC.**

In HILIC, evidence has shown that retention is achieved by partitioning in and out of a water layer surrounding the stationary phase surface. With a much less polar surface ~~TYPE-C~~ silica columns do not exhibit this same partitioning retention behavior.

Speculated local solvent displacement in ANP retention is likely to lead to faster mass transfer than partitioning in and out of a water layer. The figure below illustrates the difference in efficiency measured as height equivalent of a theoretical plate, (*HETP*) between an ANP column and a HILIC column. The significant difference in van Deemter plots suggests that the two mechanisms are very different.

See also: [What are the main differences between ANP and HILIC?](#)

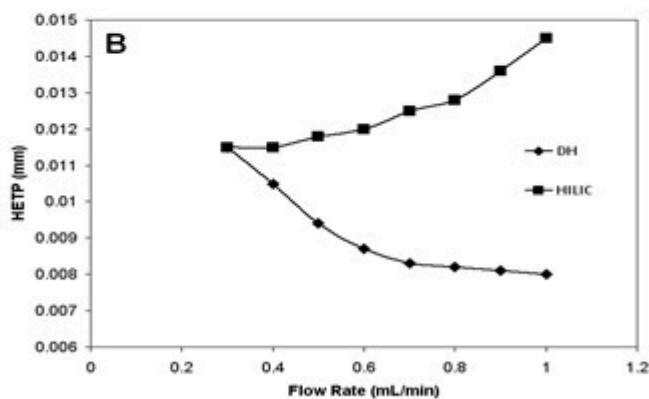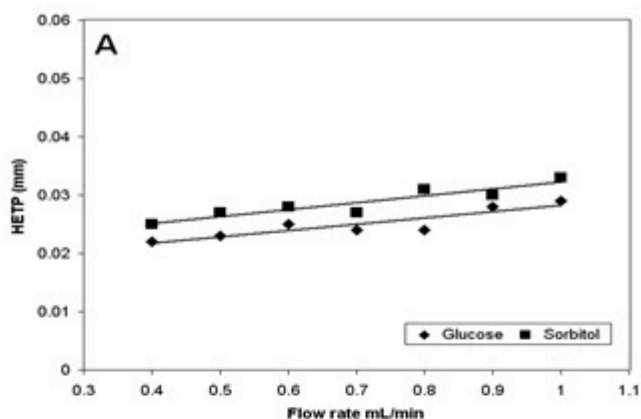

Plots of HETP versus flow rate. (A) Glucose and sorbitol on DH column (2.1 x 150 mm, particle size 4  $\mu$ m) in a 80:20 ACN/DI water + 0.1% formic acid mobile phase. (B) Comparison of commercial HILIC (4.6 x 150 mm, particle size 3.5  $\mu$ m) and DH (4.6 x 150 mm, particle size 4.0  $\mu$ m) columns for ANP retention of uracil. Mobile phase same as A.



Printed from the Chrom Resource Center  
Copyright 2025, All Rights Apply  
**MicroSolv Technology Corporation**  
9158 Industrial Blvd. NE, Leland, NC 28451

Tel: (732) 380-8900  
Fax: (910) 769-9435  
Email: [customers@mtc-usa.com](mailto:customers@mtc-usa.com)  
Website: [www.mtc-usa.com](http://www.mtc-usa.com)